

# Kongeriget Danmark

Patent application No.: PA 2003 00894

Date of filing: 17 June 2003

Applicant:  
(Name and address) Rigshospitalet  
Blegdamsvej 9  
DK-2100 København Ø  
Denmark

Title: Device for preventing dislocation of hip arthroplasty implants

IPC: -

This is to certify that the attached documents are exact copies of the above mentioned patent application as originally filed.

BEST AVAILABLE COPY



Patent- og Varemærkestyrelsen  
Økonomi- og Erhvervsministeriet

07 July 2004

*Susanne Morsing*  
Susanne Morsing

**PRIORITY DOCUMENT**  
SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH  
RULE 17.1(a) OR (b)

17 JUNI 2003

PVS

## DEVICE FOR PREVENTING DISLOCATION OF HIP ARTHROPLASTY IMPLANTS

## FIELD OF THE INVENTION

The invention relates to a method and a device for preventing dislocation of hip  
5 arthroplasty implants. The invention prevents dislocation by providing a restraining force  
on the femoral part of the implant under all movements of the leg. The invention further  
provides a method for mounting the device on a hip arthroplasty implant.

## BACKGROUND OF THE INVENTION

10 In most western countries, the typical number of total hip joint arthroplasty every year lies  
between 0,5-1 ‰ of the population. World-wide an estimated number of 1 million people  
have a total hip joint arthroplasty every year (2003), with numbers increasing. Although  
total hip joint arthroplasty is a very successful orthopaedic surgical procedure, it suffers  
from a serious drawback, namely dislocation of the hip joint. Dislocation typically occurs  
15 after a wrong movement of the leg by the patient, whereby the femoral head is drawn out  
of the cup. The causes are many, e.g. wrong or imprecise placement of the arthroplasty  
components, looseness in the surrounding tissue, of failure on the patients side to follow  
the restrictions in movements following from the surgery.

20 Dislocation after a total hip joint arthroplasty is a common adverse effect for patients  
having hip arthroplasty implants. Surveys report that 3-5 % of the patients experience a  
dislocation at some point. However, numbers as high as 15% has been reported. A  
dislocation can occur at any time in the lifetime of the arthroplasty, with an increased risk  
within the first month after the operation. It is not only a nuisance for the patient, it is also  
25 a substantial economical burden to hospitals and insurance companies.

A number of measures have been taken to avoid dislocation, including modification of the  
components to try and make the arthroplasty more stable. However, any use of locking  
mechanisms between the femoral ball and the acetabular socket has been fraught with  
30 problems. Such constrained sockets fail early because of high stresses arising from  
impingement between the socket and femoral neck. This may cause the socket to pull out  
from the bone attachment in the pelvis, or dislodge the ring lock holding the devices  
together.

35 A number of flexible constraining devices have been suggested.

US 5,755,907 describes an implantable module for use with a prosthetic joint that utilises  
a bellows and bearing with a rotating seal for encapsulating the articulating members of  
the implant. The bellows and the bearing primarily serve the purpose of containing a

lubricant to decrease the wear to the articulating parts. The implant module further serves the purpose of keeping the articulating bearing surfaces in proper alignment by providing a spring force from the metallic bellows. The bearing with the rotating seal connects the bellows and femoral neck of the implant. The rotating seal ensures free rotation of the femur in relation to the bellows.

US 6,228,122 discloses a semiconstrained net device to be attached to an acetabular cup and having a net ring around the femoral neck of the implant. The net device serves the purpose of preventing dislocation between the acetabular cup and the replacement femur.

10 The net is fixed at specific positions of the acetabular cup to provide tension only at specific positions of the hip joint. In alternatively embodiments, the net is attached directly to a point on the femoral bone in one end and in the bone adjacent to the acetabular cup in the other end. This however, is not practically possible due to the difficulties that occur while placing the bore holes correct in the acetabular rim and hereby getting the correct

15 tension of the semiconstraining device.

The net described in 6,228,122 is tightened to the cup of the adjacent bone by drawing a string of the net through a hole in the cup or bone. It is described that the tension of the net can be either pre-set or tensioned intraoperatively, presumably by knots on the string.

20 It is a disadvantage of the pre-set tension that the tension of the device can not be precisely adapted to the anatomy of the patient. It is a disadvantage that the intraoperative tensioning can not be performed in a reproducible manner.

It is a disadvantage of the above devices that the net or bellows are not fastened in fixed relation to and circumventing the femoral neck. Since the femoral neck can rotate freely around its axis without stretching of the net or bellows, these only serve as a stop for preventing the femoral head from popping out of the cup.

#### SUMMARY OF THE INVENTION

30 In the creative intellectual process leading to the present invention, the inventors have applied their detailed expertise within the field of hip arthroplasty combined with a dynamical and mechanical approach. This has given a thorough understanding of the dynamical aspects of hip dislocation in arthroplasty implants.

35 Dislocation may occur at specific positions of the joint and during special combinations of movements of the leg. Hence, in order for an anti-dislocation device to function properly, it should prevent the joint in reaching positions where dislocations are likely to occur by restraining movements typically leading to those positions. Alternatively the device should

provide an extra securing of the femoral head in the cup at the positions where dislocations are likely to occur. Both these demands may be met by a device which

- a) provides a restraining force opposing movements typically leading to positions where dislocations are likely to occur, and which
- 5 b) provides an extra securing force for holding the femoral head in the cup when the leg is at positions where dislocations are likely to occur.

The device according to present invention provides these functions whilst representing a substitution of the anatomic and physiologic fibrous capsule. In order not to reduce the freedom of movement of the patient's leg, the restraining and securing forces should  
10 preferably increase with the amplitude of the movement.

In this description, a hip arthroplasty implant comprises at least the following components, an acetabular cup to be mounted in the acetabular cavity of a pelvis, a femoral stem to be mounted in the proximal end of a femoral bone and having a femoral neck, and a femoral  
15 head to be mounted on the femoral neck and to be situated in a receiving cavity of the acetabular cup. These components will be referred to throughout the text.

In general, any movement of a physical object can be resolved into a translation of the object to obtain its new position followed by a rotation around a properly chosen axis to  
20 obtain its new orientation. In a similar fashion, any normal movement of a hip joint can be resolved into two rotations around perpendicular axes; a rotation around a first axis through the centre of the femoral neck followed by a rotation around a second axis through the centre of the femoral head, which axis is perpendicular to the first axis. In the present specification, rotation around the first axis is referred to as axial rotation, whereas  
25 rotation around the second axis is referred to as planar rotations (as the femoral neck spans a plane during this). Almost all movements of the leg include combinations of axial and planar rotations.

In a first aspect, the invention provides a device for preventing dislocation of a hip  
30 arthroplasty implant, the device comprising

- a tubular collar having a first open end having a first rim and a second open end having a second rim,
- 35 - first fastening means for fastening the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup, and
- second fastening means for fastening the second rim to the femoral neck,

the device being characterised in that the second fastening means is adapted to fasten the second rim in fixed relation to and circumventing the femoral neck to prevent longitudinal movement of the second rim along the femoral neck and rotational movement of the second rim around the femoral neck.

5

It is of importance that the second rim is fastened in fixed relation to the femoral neck and that it is fastened to circumvent the femoral neck. The fixed fastening means that the femoral neck can not rotate without twisting the collar. Thus, any movement involving axial rotations will twist the tubular collar and thereby also stretch it along its longitudinal axis. Thereby, the tubular collar will execute a force restraining the movement of the femoral neck and a force pulling the femoral head towards the receiving cavity of the cup. These forces arise because the longitudinal stretching generates a force which can be resolved into two perpendicular components. A first component is perpendicular to the neck and represents a force restraining the movement. A second component is parallel to the neck and represents a securing force for holding the femoral head in the cup (please refer to Figure 7). The twisting of the collar has another important property. If the movement involves only planar rotation, the collar is stretched in one side and slacked in the opposite side. However, as most movements of the leg involve both axial and planar rotations, the collar will be stretched/slacked and twisted at the same time. The twisting of the collar will tighten the slacked side of the collar whereby this part will also contribute with a securing force component. In the devices described in the prior art, the femoral neck can rotate freely, and the net/bellows are not twisted. Therefore, it is an important feature that the second rim is fastened in fixed relation to the femoral neck.

25 As the forces work on the femoral neck, and not the head itself, it is important that they work on all sides of the neck at the same time. If not, the total resulting securing force component may be asymmetric resulting in a skew pull of the neck towards the cup. Therefore, it is an important feature that the second rim is fastened so as to circumvent the femoral neck.

30

The tubular collar may be a mesh woven by e.g. cross-linked HMDPE fibres in the form of an open stocking. The fabric of the mesh preferably consists of bioacceptable material. To provide the longitudinal stretching force, the tubular collar is preferably elastic in at least a longitudinal direction. The elasticity should be chosen so that the collar is stretched without tearing by the forces in play when the device is mounted on a grown up human being. Further, the tubular collar may be elastic in a radial direction. The elastic properties of the mesh are related to the weaving technique used in the fabric.

35

In alternative embodiments, the tubular collar may be a tubular biocompatible rubber membrane, or a bellows comprising metal springs. In all embodiments, the tubular collar preferably has the shape of a truncated cone.

- 5 The first and second fastening means preferably comprise first and second rings attached to the first and the second rim. The first ring may have one or more protrusions on, or incisions in, a first surface so that it can be assembled with a surface part of the acetabular cup, or with a flange to be fixed on the acetabular cup, having at least one corresponding incision or protrusion.

10

- In a preferred embodiment, the second ring attached to the second rim has a slot for receiving a clamp formed as an open ring to be inserted in said slot. The femoral neck, or a flange to be fixed on the femoral neck, has an outer circumference with a shape corresponding to a shape of the inner circumference of said clamp. By mounting the  
15 second ring on the femoral neck (or the flange), the clamp can be inserted in the slot to fix the ring on the femoral neck.

- Alternatively, the second ring may have one or more protrusions on or incisions in an internal circumference so that it can be mounted on the femoral neck, or a flange to be  
20 fixed on the femoral neck, having at least one corresponding incision or protrusion around its outer circumference.

- This will allow for each of the end of the tubular collar to be fixed at several different positions so that the collar can be mounted in a position where it is not twisted.

25

- In an alternative embodiment, the second fastening means comprises a ring attached to the second rim, which ring can be fixedly mounted around the femoral neck by shrink fitting. Alternatively, the second fastening means comprises a ring attached to the second rim, which ring can be fixedly mounted around the femoral neck by at least one bolt,  
30 screw, clamp or clip.

In a second aspect, the invention provides a method for stabilisation of a hip arthroplasty implant with a device for preventing dislocation of the hip arthroplasty implant,

- 35 the device for preventing dislocation comprising an elastic tubular collar having a first open end to be mounted in fixed relation to and encircling the receiving cavity of the acetabular cup, and a second open end to be mounted in fixed relation to and circumventing the femoral neck,

the method preventing dislocation of the hip arthroplasty implant by the steps of

- providing a joint of a hip implant in a neutral position with a tubular collar being fixedly mounted, and
- moving the joint of the hip implant away from the neutral position,
- 5 - executing a force restraining the movement of the femoral neck and a force pulling the femoral head towards the receiving cavity of the acetabular cup.

The movements of the joint away from the neutral position may be described by the previously defined axial and planar rotations. Alternatively, the movements may be  
10 described by the movements of the leg using the anatomical terms from the following definitions:

- Sagittal Plane: A vertical plane extending in an antero-posterior direction dividing the body into right and left parts.
- Frontal Plane: A vertical plane at right angles to the sagittal plane that divides the body  
15 into anterior and posterior portions.
- Transverse Plane: A transverse plane at right angle to the long axis of the body, same as horizontal plane.
- Extension: A movement at a joint resulting in separation of two ventral surfaces (as opposed to flexion).
- 20 - Flexion movement: A movement at a joint resulting in approximation of two ventral surfaces (as opposed to extension).
- Abduction: A movement from a midline (as opposed to adduction).
- Adduction: A movement toward a midline (as opposed to abduction).

25 The movement of the leg may be described by the following movements:

- flexion movement in a sagittal plane,
- extension movement in a sagittal plane,
- adduction movement in a frontal plane,
- abduction movement in a frontal plane,
- 30 - external rotation in a transverse plane,
- internal rotation in a transverse plane,

or any combination thereof.

In the experience of the inventors, dislocation is especially likely to occur under  
35 movements that are similar but inverse to those used by surgeons to relocate dislocated joints. These may be described as a combination of flexion and inward rotation and perhaps adduction.

The forces in play under movements of the joint of the hip implant will be described in larger detail elsewhere in the specification.

In a third aspect, the invention provides a method for mounting an device for preventing  
5 dislocation on a hip arthroplasty implant,

the device for preventing dislocation comprising

- a tubular collar having a first open end having a first rim and a second open end having a second rim, the tubular collar being elastic in at least a longitudinal direction,
- 10 - first fastening means for fastening of the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup, and
- second fastening means for fastening of the second rim in fixed relation to and circumventing the femoral neck,

15 the method comprising the steps of:

- mounting the tubular collar to the femoral neck and positioning the femoral head in the acetabular cup with the leg and hereby the femur containing the femoral stem situated anatomically,
- positioning the leg and hereby the femur containing the femoral stem in a neutral  
20 position,
- fastening the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup with the first fastening means,
- fastening the second rim in fixed relation to and circumventing the femoral neck with the second fastening means,

25 wherein the steps of fastening the first or second rim to the first or second fastening means, respectively, comprises the step of uniformly tightening or stretching the tubular collar, so that the tubular collar during movement of the leg exerts a force restraining the movement of the femoral neck and a force pulling the femoral head towards the receiving cavity of the acetabular cup.

30

The position of the femoral component during mounting of the device is important for the performance. Preferably, the tubular collar should be uniformly tight when the leg is in a neutral position, so as to act upon movements towards positions where dislocations are likely to occur. However, the leg has many natural position (when the patient is standing,  
35 lying, sitting etc.), and an appropriate position should be chosen. When an appropriate neutral position is chosen, attention should be paid to acetabular inclination and anteversion and leg length, among other things.



As described in relation to the first aspect, the first and second fastening means preferably comprise first and second rings attached to the first and the second rim. These rings are to be attached at the acetabular cup and at the femoral neck, respectively. As the femoral head is larger than the circumference of the second ring, the second ring is preferably  
5 mounted on the femoral neck before putting on the femoral head. Optionally, only the second ring is mounted, in which case the collar can be fastened to the second ring at a later stage.

#### BRIEF DESCRIPTION OF THE DRAWINGS

10 Figure 1 shows a hip with a typical hip arthroplasty implant.

Figure 2 is an illustration of a hip arthroplasty implant mounted with a device for preventing dislocating according to a preferred embodiment of the invention.

15 Figure 3A and B illustrates the first fastening means for fastening the device according to the invention to the acetabular cup.

Figure 4A, B, and C illustrates the second fastening means for fastening the device according to the invention to the femoral stem.

20

Figure 5 shown a planar rotation movement of a hip arthroplasty implant with a device for preventing dislocating according to the invention.

Figure 6 shown an axial rotation movement of a hip arthroplasty implant with a device for  
25 preventing dislocating according to the invention.

Figure 7 illustrates the forces from the tubular collar of the device under the movements illustrated in Figures 5 and 6.

30 Figure 8 is a graph showing the response of a spring and a rubber band.

#### DETAILED DESCRIPTION OF THE INVENTION

Figure 1 shows a typical hip arthroplasty implant 1 with an acetabular cup 2 cemented in the acetabular cavity of the human pelvis 3, a femoral stem 4 mounted in the proximal  
35 end of a human femoral bone 5, the femoral stem having a femoral neck 6, and a femoral head 7 mounted on the femoral neck 6 and situated in a receiving cavity of the acetabular cup 2.

Also shown in Figure 1 is the first axis 10 of the femoral neck 6. Arrow 11 illustrates axial rotations while arrow 12 illustrates planar rotation according to the previous definitions.

Figure 2 shows an embodiment of the device 20 for preventing dislocation according to the present invention. The device 20 has a tubular collar 21 made from a woven mesh. The device 20 has a first fastening means 22 to fasten a first rim 23 of a first open 24 end of the collar 21 to the acetabular cup 2. Similarly, the device 20 has a second fastening means 25 to fasten a second rim 26 of a second open 27 end of the collar 21 to the femoral neck 6.

10

The fastening means 22 and 25 provides the fixation of the collar to the cup and the stem. The collar can in principle be fastened to either the cup or stem prior to the operation. However, typically the collar can cause inconvenience during mounting of the stem and cup in the patient. For this reason, the mounting and final fastening of the collar will be done at the end of the hip arthroplasty operation. During the final fastening, the tubular collar should be uniformly tight and straight (no twisting) with the leg in a neutral position. It is therefore important that the fastening means can fix the collar at several positions around the first axis 10.

20 Figure 3A and B illustrates a preferred embodiment of the first fastening means 22. In Figure 3A, the first fastening means 22 consist of a ring 30 attached to the first, wider rim 23 of the tubular collar 21 (see Figure 3B). The ring 30 has a number of holes or incisions 32 to fit a number of protrusions 35 on a part 34 of the acetabular cup 2 facing the ring 30. The incisions 32 and protrusions enables the ring 30, and thereby the collar 21, to be securely fastened in a number of different positions around the first axis 10 (see Figure 1). The ring 30 further has two or more holes 33 for screws or bolts to fix the ring 30 to the part 34. Figure 3B illustrates the ring 30 fastened on the acetabular cup 2 with screws 36.

Figure 4A, B and C illustrates a preferred embodiment of the second fastening means 25. The second fastening 25 consist of a ring 40 attached to the second, narrower rim 26 of the tubular collar 21. The ring 40 is to be fastened on the femoral neck 6. As shown in Figure 4B, a stationary flange 48 is fixated on the femoral neck 6. The flange 48 has incisions 49 representing the positions around the first axis 10 (see Figure 1) on which the collar 21 can be fastened. To fasten the ring 40 on the flange 49, the ring 40 is slit over the flange 49 at the desired position around the first axis. The second fastening also includes a locking clamp 44 shown in Figure 4C. The clamp 44 fits in a slot 42 in the ring 40 (see Figure 4A). The straight side parts of the clamp 44 fits the width of the slot 42, so that the clamp can be inserted in the slot without clearance. An outer perimeter of the flange 48 of Figure 4B fits an inner perimeter of the clamp 44. The clamp has a protrusion

46 on its inner perimeter corresponding to the incisions 49 in the flange. The clamp 44 also has a pin 45 for inserting and removing the clamp. The ring is locked in the desired position by insertion of the clamp 44 in the slot 42.

- 5 When the joint of the implant undergoes planar rotations, one side of the collar is stretched as illustrated in Figure 5. The side of the collar opposite to the stretched side will be slacked. If the collar is a mesh as shown in Figure 5, then stretching the collar means stretching individual strings in the mesh. As illustrated in Figure 7, the stretching of a string produces a stretching force  $F_{\text{stretch}}$  having a component  $F_{\text{restrain}}$  restraining the planar
- 10 rotation and component  $F_{\text{secure}}$  pulling the femur towards the pelvis and thereby securing the femoral head in the cup. The same forces come into play if a continuous material such as a rubber sheet forms the collar.

- As described previously, axial rotations as illustrated in Figure 6 will twist the tubular collar
- 15 because the femoral neck can not rotate without the collar. As the distance between the first and second fastening means 22 and 25 does not change, the twisting stretches the individual strings in the mesh, and thereby also the collar along its longitudinal axis. Thus, the forces of Figure 7 come into play as for the planar rotation of Figure 5.

- 20 When the movement is a combination of planar and axial rotations, as most normal movements are, the stretching/slacking of Figure 5 is combined with the twisting of Figure 6. Thus, the strings on both the stretched and the slacked side of Figure 5 will be stretched due to the twisting. Thereby, the strings on the slacked side will not be slacked, only less stretched than the strings on the stretched side. The force components  $F_{\text{restrain}}$  and  $F_{\text{secure}}$  of
- 25 Figure 7 will increase due to this combined effect, so that
- the femoral head will be held even more securely in the cup, and
  - the motion will be restrained even further, minimising the risk for the leg to move to a dislocating position.

Thus, the twisting of the collar enhances the anti-dislocation effect of the device.

- 30 As mentioned previously, the restraining and securing forces provided by the collar may increase with the amplitude of the movement. This will increase the freedom of movement of the leg for small amplitudes while increasing the restraining and securing forces for large amplitudes. The response of the collar depends on its elasticity, which depends on
- 35 the applied material and the weave of the mesh.

The spring force from a typical metal spring will increase linearly with the distance in most of its dynamical range. This is illustrated by the curve 81 in the graph 80 having the spring/elastic force  $F$  along the principal axis and the distance  $d$  along the secondary axis.

some deviation from the curve 81 will occur when the spring is close to fully stretched. Elastic materials such as rubber have a different response. Here, the force increases nonlinearly with the distance of extension. Curve 82 in Figure 8 shows the response of a normal rubber band.

5

In a preferred embodiment, the tubular collar response with a force which increase nonlinearly with an amplitude of a movement of the femoral neck. In another embodiment, the tubular collar response with a force which increase at least substantially linearly with an amplitude of a movement of the femoral neck.

## CLAIMS

1. A device for preventing dislocation of a hip arthroplasty implant, the hip arthroplasty  
5 implant comprising an acetabular cup to be mounted in the acetabular cavity of a pelvis, a femoral stem to be mounted in the proximal end of a femoral bone and having a femoral neck, and a femoral head to be mounted on the femoral neck and to be situated in a receiving cavity of the acetabular cup,
- 10 the device for preventing dislocation represents a substitution of the anatomic and physiologic fibrous capsule and comprises
- a tubular collar having a first open end having a first rim and a second open end having a second rim,
  - 15 - first fastening means for fastening the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup, and
  - second fastening means for fastening the second rim to the femoral neck,
  - 20 the device being characterised in that the second fastening means is adapted to fasten the second rim in fixed relation to and circumventing the femoral neck to prevent longitudinal movement of the second rim along the femoral neck and rotational movement of the second rim around the femoral neck.
  - 25
2. The device according to any of the preceding claims, wherein the tubular collar is elastic in at least a longitudinal direction.
3. The device according to any of the preceding claims, wherein the tubular collar is elastic  
30 in at least a radial direction.
4. The device according to any of the preceding claims, wherein the tubular collar is an elastic mesh.
- 35 5. The device according to any of the preceding claims, wherein the first fastening means comprises a ring attached to the first rim, the ring having one or more protrusions on or incisions in a first surface, and wherein an accessible surface part of the acetabular cup, or of a flange to be fixed on the acetabular cup, has at least one corresponding incision or protrusion.

6. The device according to any of the preceding claims, wherein the second fastening means comprises a ring attached to the second rim, the ring having one or more protrusions on or incisions in an internal circumference, and wherein the femoral neck or a flange to be fixed on the femoral neck has at least one corresponding incision or protrusion around its outer circumference.

7. The device according to any of the preceding claims, wherein the second fastening means comprises a ring attached to the second rim, the ring having a slot, and a clamp formed as an open ring to be inserted in said slot, and wherein the femoral neck, or a flange to be fixed on the femoral neck, has an outer circumference with a shape corresponding to a shape of the inner circumference of said clamp. .

8. A method for stabilisation of a hip arthroplasty implant with a device for preventing dislocation of the hip arthroplasty implant,

the hip arthroplasty implant comprising an acetabular cup mounted in the acetabular cavity of a pelvis, a femoral stem mounted in the proximal end of a femoral bone and having a femoral neck, and a femoral head to be mounted on the femoral neck and to be situated in a receiving cavity of the acetabular cup,

the device for preventing dislocation comprising an elastic tubular collar having a first open end to be mounted in fixed relation to and encircling the receiving cavity of the acetabular cup, and a second open end to be mounted in fixed relation to and circumventing the femoral neck,

the method preventing dislocation of the hip arthroplasty implant by the steps of

- providing a joint of a hip implant in a neutral position with a tubular collar being fixedly mounted, and
- moving the joint of the hip implant away from the neutral position,
- executing a force restraining the movement of the femoral neck and a force pulling the femoral head towards the receiving cavity of the acetabular cup.

9. The method according to claim 8, wherein the movement of the joint is chosen from a group of movements containing:

- flexion movement in a sagittal plane,
- extension movement in a sagittal plane,
- adduction movement in a frontal plane,
- abduction movement in a frontal plane,

- external rotation in a transverse plane,
  - internal rotation in a transverse plane,
- and any combination thereof.

- 5 10. The method according to claim 8, wherein the movement of the joint is chosen from:
- axial rotation around a longitudinal axis of the femoral neck,
  - planar rotations where the angle between the femoral neck and the acetabular cup changes,
  - combinations of axial and planar rotations, and
- 10 - any translation.

11. The method according to claim 8, wherein the force restraining the movement of the femoral neck increase proportionally to an amplitude of the movement.

- 15 12. The method according to claim 8, wherein the force restraining the movement of the femoral neck increase nonlinearly with an amplitude of the movement.

13. A method for mounting an device for preventing dislocation on a hip arthroplasty implant,

20

the hip implant comprising an acetabular cup mounted in the acetabular cavity of a pelvis, a femoral stem mounted in the proximal end of a femoral bone and having a femoral neck, and a femoral head to be mounted on the femoral neck and to be situated in a receiving cavity of the acetabular cup,

25

the device for preventing dislocation comprising

- a tubular collar having a first open end having a first rim and a second open end having a second rim, the tubular collar being elastic in at least a longitudinal direction,
  - first fastening means for fastening of the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup, and
- 30 - second fastening means for fastening of the second rim in fixed relation to and circumventing the femoral neck,

the method comprising the steps of:

- 35 - mounting the tubular collar to the femoral neck and positioning the femoral head in the acetabular cup with the leg containing the femoral stem situated anatomically,
- positioning the leg in a neutral position,
  - fastening the first rim in fixed relation to and encircling the receiving cavity of the acetabular cup with the first fastening means,

- fastening the second rim in fixed relation to and circumventing the femoral neck with the second fastening means,

wherein the steps of fastening the first or second rim to the first or second fastening means, respectively, comprises the step of uniformly tightening or stretching the tubular

- 5 collar, so that the tubular collar during movement of the leg exerts a force restraining the movement of the femoral neck and a force pulling the femoral head towards the receiving cavity of the acetabular cup.

14. The method according to claim 9, wherein the step of applying the tubular collar to the
- 10 hip arthroplasty implant comprises the steps of mounting the tubular collar on the femoral neck so that the second rim encircles of the femoral neck and thereafter mounting the femoral head on the femoral neck.



1/4

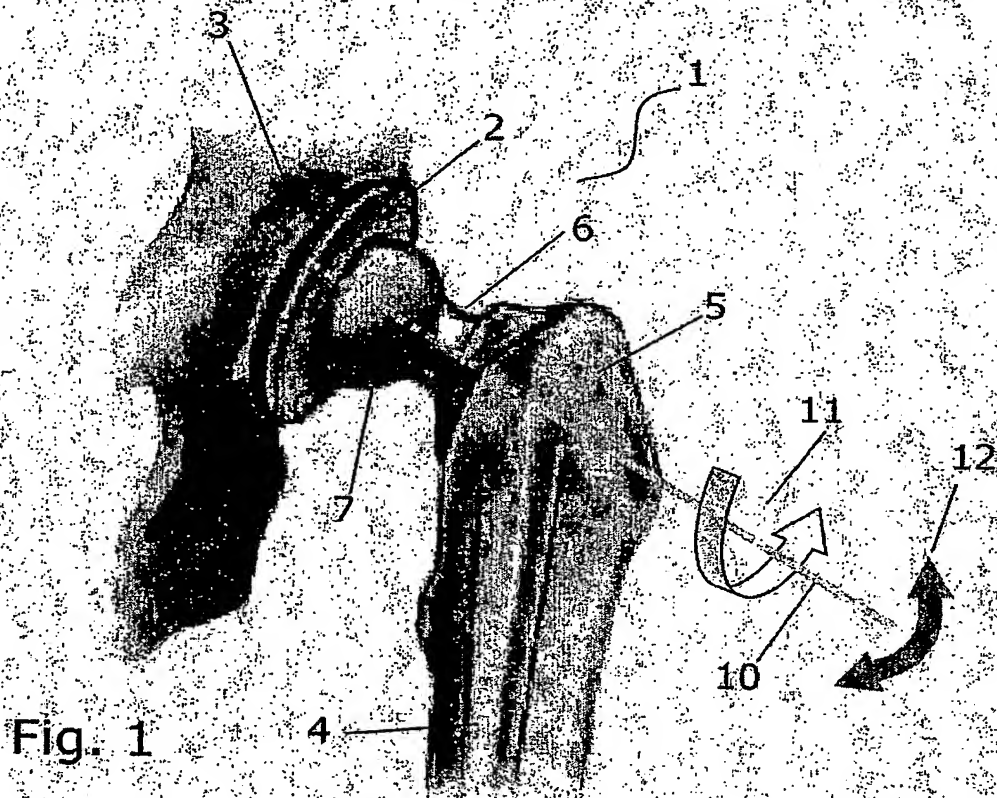


Fig. 1

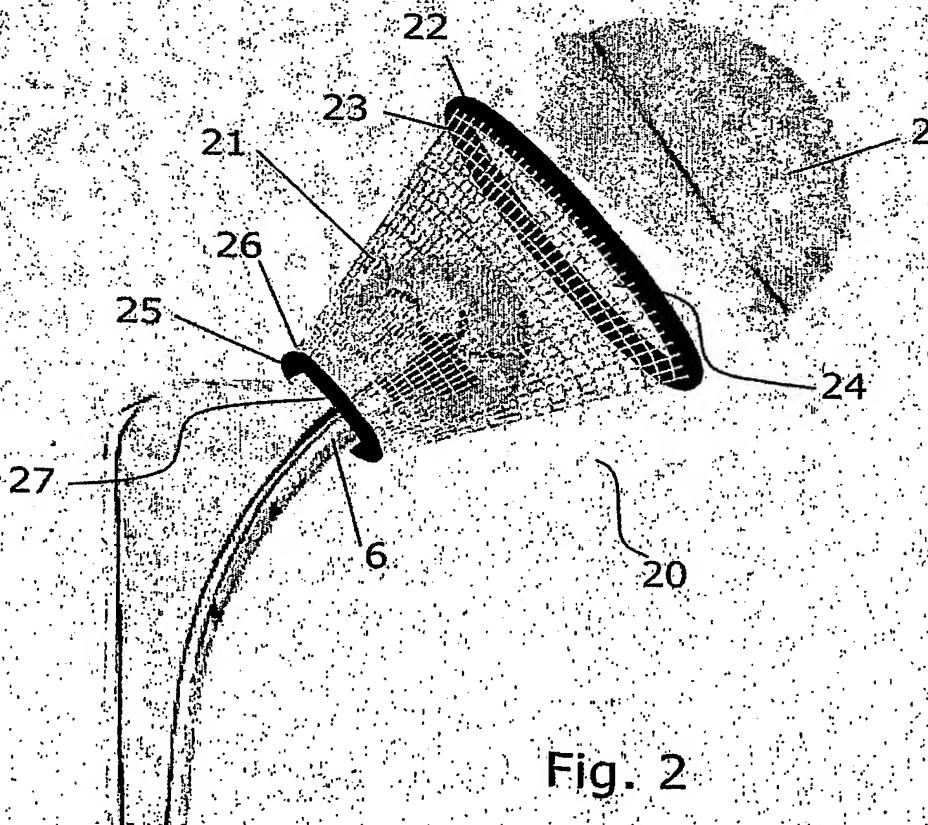


Fig. 2

2/4

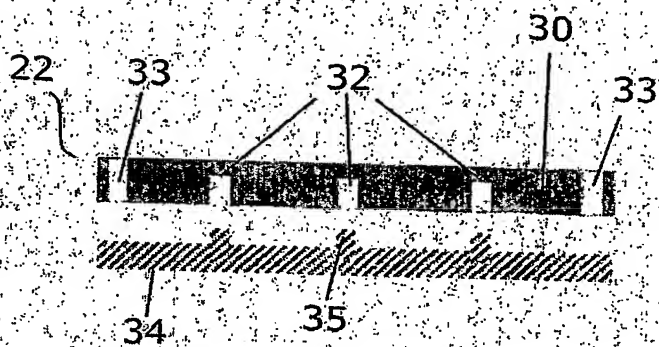


Fig. 3A

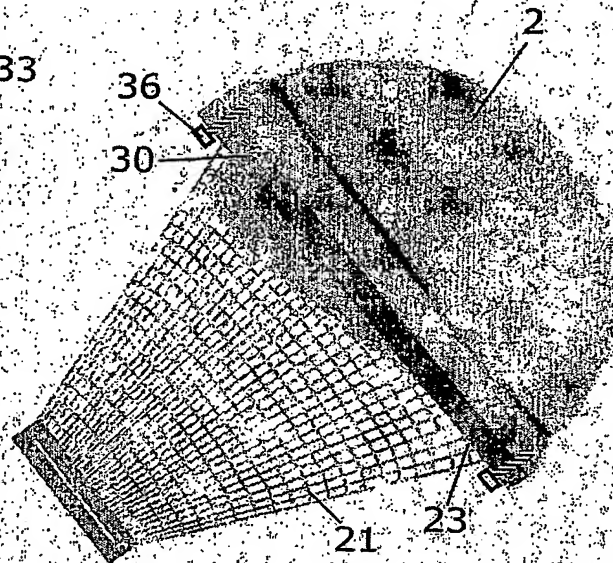


Fig. 3B

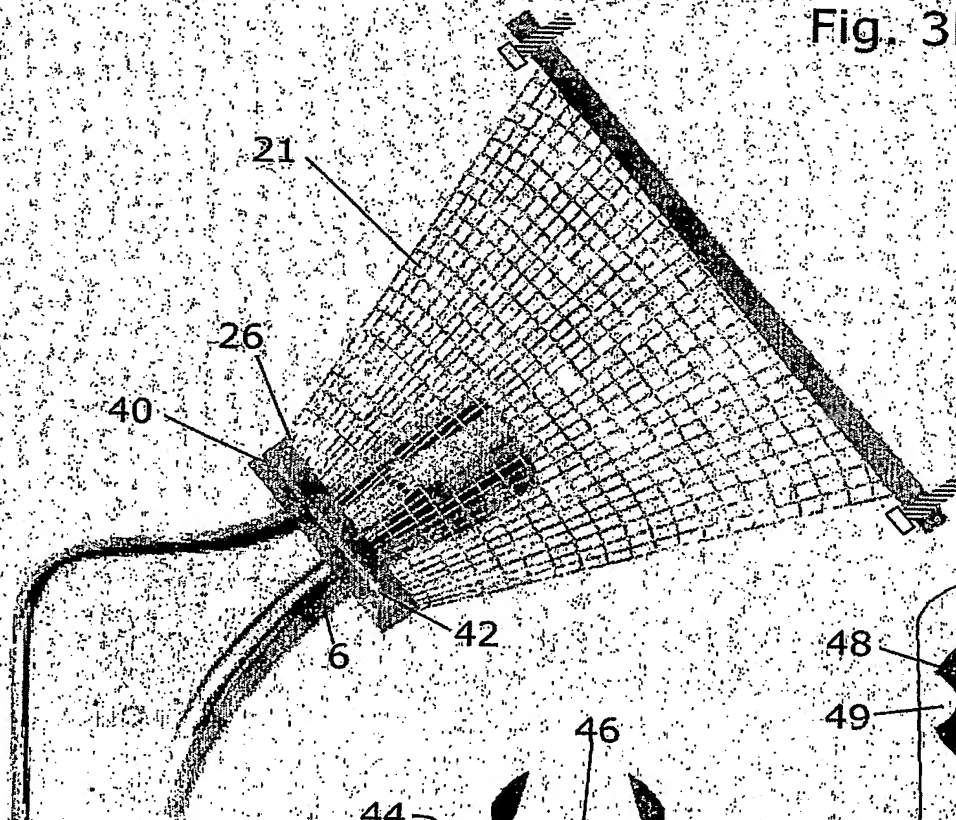


Fig. 4A

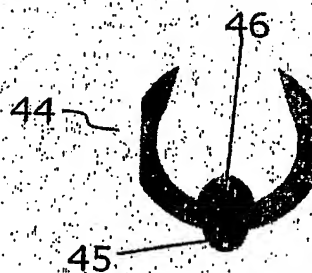


Fig. 4C

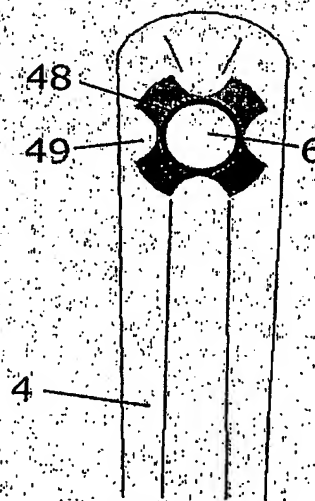


Fig. 4B

3/4

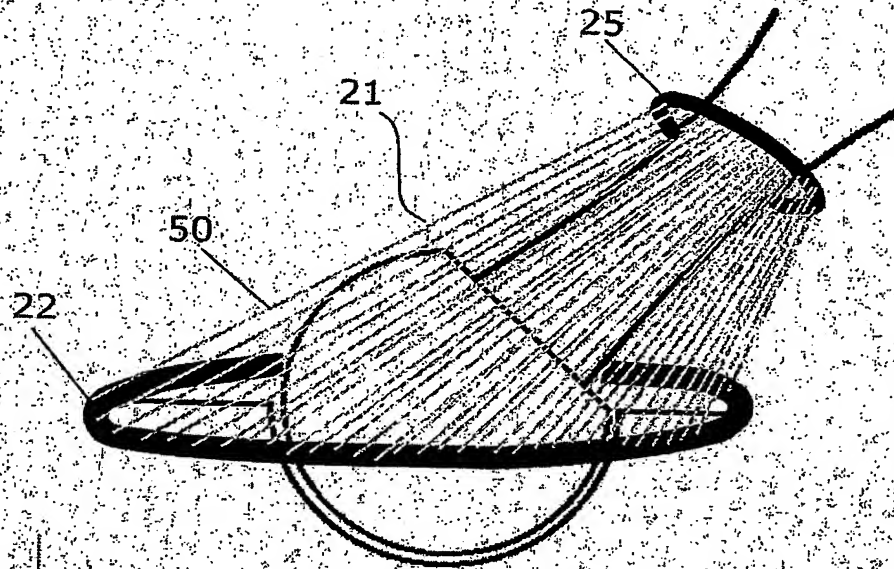


Fig. 5

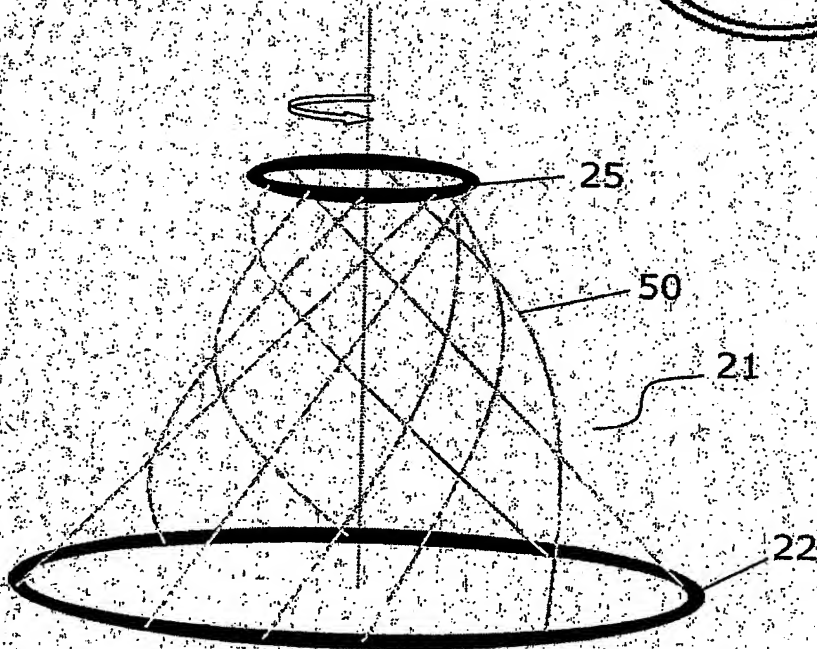


Fig. 6

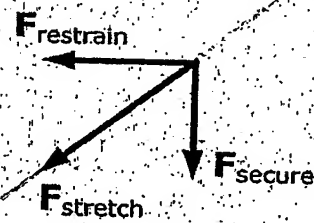


Fig. 7

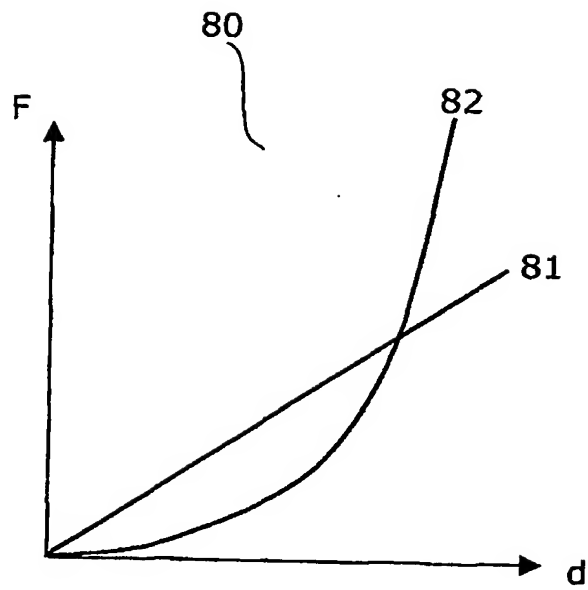


Fig. 8

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☒ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**